


Title : IMG1

 Instrument : JCM-6000
 Volt : 15.00 kV
 Mag. : x 220
 Date : 2020/05/04
 Pixel : 512 x 384

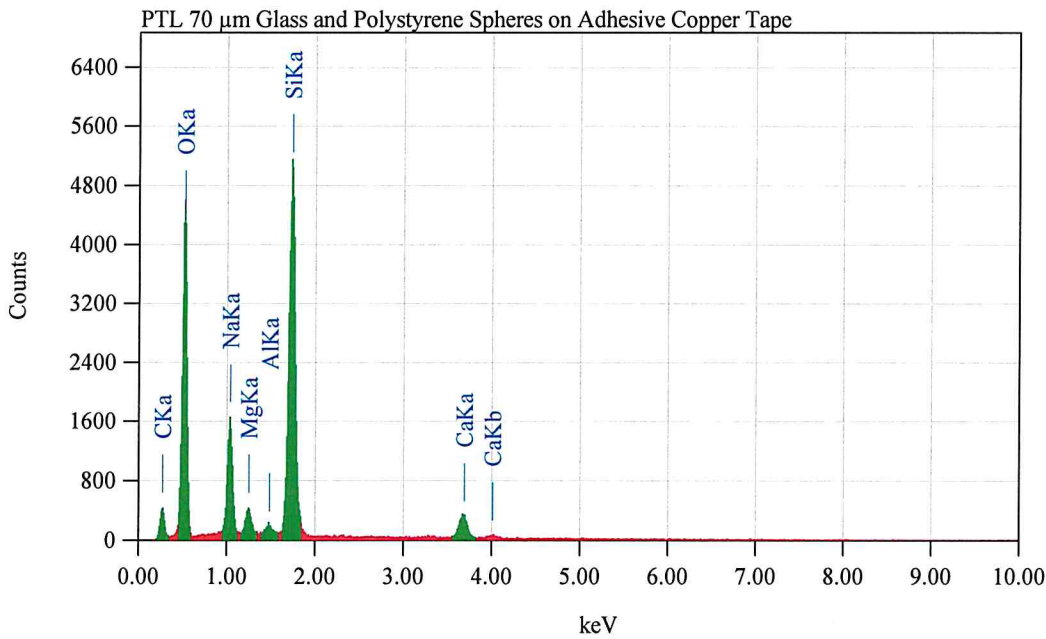

Acquisition Parameter
 Instrument : JCM-6000
 Acc. Voltage : 15.0 kV
 Probe Current: 1.00000 nA
 PHA mode : T3
 Real Time : 31.23 sec
 Live Time : 30.00 sec
 Dead Time : 3 %
 Counting Rate: 3763 cps
 Energy Range : 0 - 20 keV

ZAF Method Standardless Quantitative Analysis

Fitting Coefficient : 0.0951

Element	(keV)	Mass%	Sigma	Atom%	Compound	Mass%	Cation	K
C K	0.277	17.78	0.13	24.63				3.7178
O K	0.525	57.55	0.25	59.86				62.4128
Na K*	1.041	7.61	0.07	5.51				6.8691
Mg K*	1.253	1.42	0.04	0.97				1.2681
Al K*	1.486	0.35	0.02	0.22				0.4156
Si K*	1.739	13.91	0.08	8.24				21.7786
Ca K*	3.690	1.38	0.03	0.57				3.5381
Total		100.00		100.00				